



TOXOCARA IgG CELISA

INTENDED USE AND PRINCIPLE OF THE TEST

This test is designed to detect and measure antibodies to *Toxocara canis* excretory-secretory (ES) antigen produced during infection in humans. The Toxocara IgG CELISA is a solid phase enzyme immunoassay. Antibody is bound by the *Toxocara* ES antigen coated on the inner surface of the test strip. Peroxidase-conjugated antibody to human IgG is added and reacts with bound antibody. A chromogenic substrate for peroxidase is added. If antibody to *Toxocara* is present there is a reaction which results in the development of a blue colour, which is in proportion to the serum level of the antibody. Addition of stopping solution changes the blue colour to yellow.

CONTENTS OF THE KIT

TXMW	Celisa Plate – 1 x 96 wells - (single use only)	2 plates
TXPC	Positive Control	0.2mL
TXNC	Negative Control	0.2mL
TXPO	Enzyme Conjugate (200x)	0.2mL
TXPT	PBS/Tween (20x)	110mL
TXSC	Substrate Chromogen (TMB) (20x)	1.5mL
TXSB	Substrate Buffer	24mL
TXSS	Stopping Solution	12mL


All components should be stored at 2-8°C, and are supplied ready for use. Expiry dates are clearly marked on each kit component and on the box and do not change once opened.

MATERIALS REQUIRED BUT NOT PROVIDED

- Micropipettes and tips
- Clean glassware or plastic containers for solutions.
- Humid chamber
- ELISA washer
- Spectrophotometer to read absorbance at a single wavelength of 450nm

DIAGRAM FOR USE

Use Cellabs Instructions for Use Insert contained in kit when performing test, and refer to Material Safety Data Sheet (MSDS) for further information.

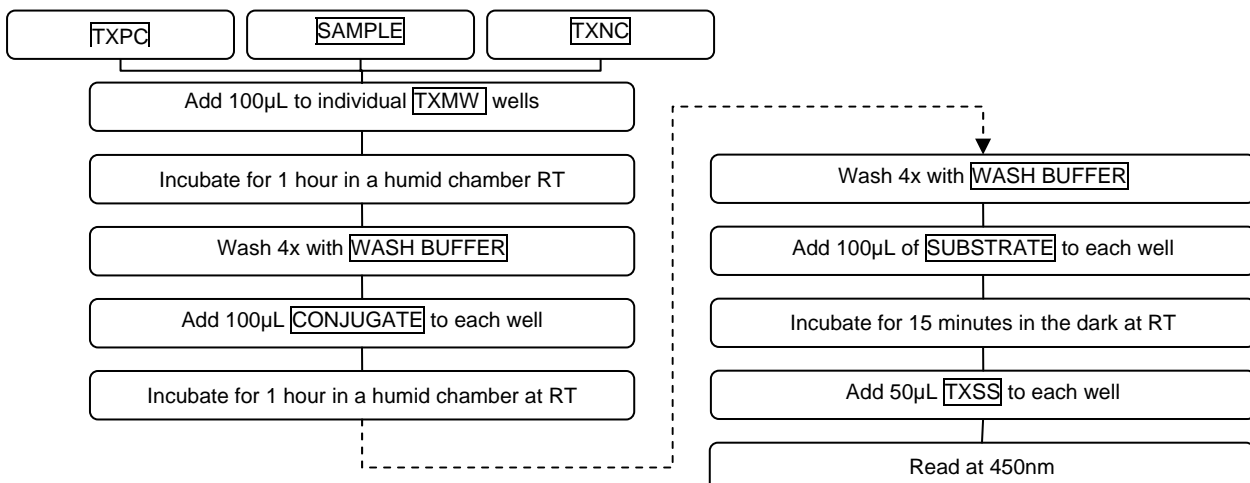

READING AND INTERPRETATION OF RESULTS AND DIAGNOSIS

Samples may be read visually or photometrically. Visually, samples giving the same or less colour than the negative control are considered negative. Samples giving colour greater than the negative control, similar to the positive control, are considered positive. Using a spectrophotometer, negative samples should give an optical density below a certain level and positive samples should give an optical density above a certain level. Please refer to the kit insert for detailed information.



Cellabs Product Profile

PERFORMANCE DATA FOR TOXOCARA IgG CELISA

Sensitivity/Specificity

B	n = 92 serum samples. Toxocara IgG CELISA versus another ELISA.	Sensitivity: 90% Specificity: 94%
---	---	--------------------------------------

Repeatability

3 Positive samples and a Negative sample were tested in replicates of 8, by two different operators. The coefficient of variation for repeatability ranged between 3.03% and 9.51%, with an average of 7.11% for Positive samples. The average coefficient of variation for repeatability for the Negative sample was 9.36%.

Reproducibility

3 Positive samples and a Negative sample were tested in replicates of 8, by two different operators. The coefficient of variation for reproducibility ranged between 6.71% and 8.12%, with an average of 7.24% for Positive samples, and a coefficient of variation of 9.49% for the Negative sample.

For Ordering Assistance:

See Your Local Distributor:

OR

Cellabs Pty Ltd
Unit 7, 27 Dale Street (PO Box 421)
Brookvale, NSW 2100 Australia
Tel: +61 2 9905 0133 Fax: +61 2 9905 6426
Web: <http://www.cellabs.com.au>
Email: sales@cellabs.com.au



Authorised Representative in the European Community:

MDCI Ltd
Arundel House
1 Liverpool Gardens
Worthing, West Sussex BN11 1SL
United Kingdom